

Standard Differential Thermal Relief (DTR)

This configuration is acceptable for liquid service.


BODY BLEED VALVE is only for the purposes of manually venting the body cavity and DBB testing.

When not being used for bleeding, the body bleed valve should be closed and the outlet should be plugged.

UPSTREAM ISOLATION VALVE must be left open for cavity relief to function.

It should only be closed for maintenance and leakage management in the event of damage.

Directionality characteristics of valve are shown below.

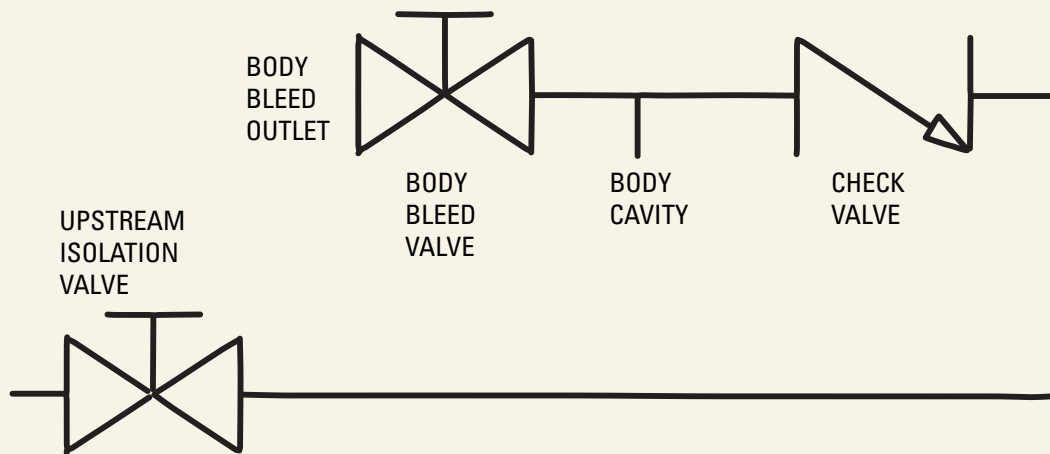

Sealing of valve seats with different isolation settings.

